


*I-V of Micron Oxygenated barrel detectors after  $3 \times 10^{14} \text{ p. cm}^2$*



*I-V of Micron standard barrel detectors after  $3 \times 10^{14} \text{ p. cm}^2$*

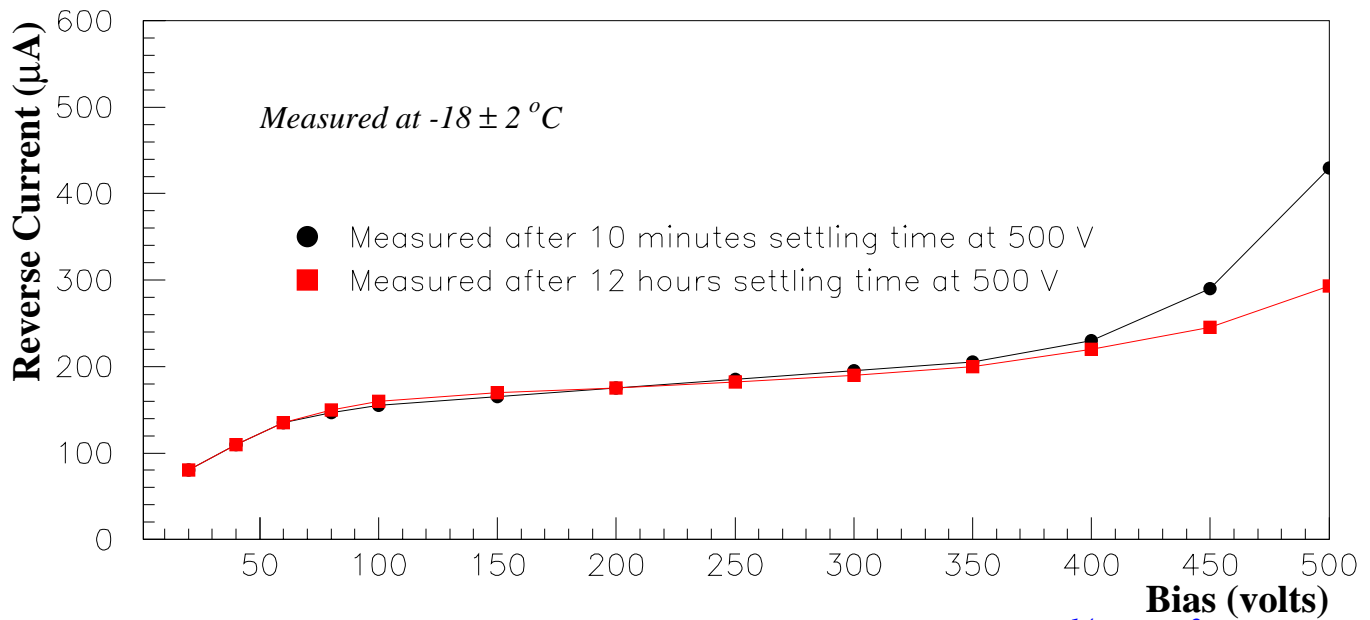